


SPECIALTY HPLC COLUMNS

Polymer AAA 8µm Column: Amino Acid Analysis with Ninhydrin Detection

Protein Feedstuff Hydrolyzate Standard (250 µmol/l)

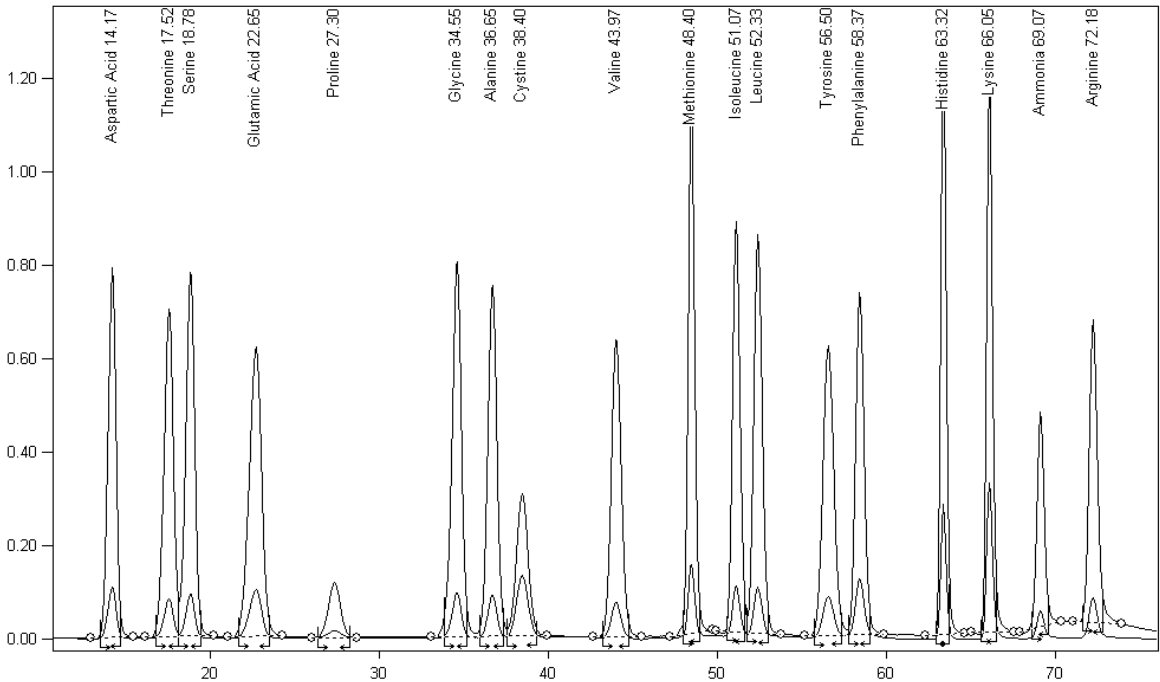

Column: Watrex 250x4 mm Polymer AAA 8µm
Flow rates: 0,3 ml/min (buffer), 0,2 ml/min (reagent)
Mobile phase: composition and gradient program on request
Column temperature: gradient program on request
Detection: 570/440 nm